



# A label-free fluorimetric detection of biothiols based on the oxidase-like activity of Ag<sup>+</sup> ions



Ru Li<sup>a</sup>, Cuihua Lei<sup>a</sup>, Xian-En Zhao<sup>a</sup>, Yue Gao<sup>a</sup>, Han Gao<sup>a</sup>, Shuyun Zhu<sup>a,b</sup>, Hua Wang<sup>a,b,\*</sup>

<sup>a</sup> Shandong Provincial Key Laboratory of Life-Organic Analysis, College of Chemistry and Chemical Engineering, Qufu Normal University, Qufu City, Shandong Province 273165, China

<sup>b</sup> Institute of Medicine and Materials Applied Technologies, Qufu Normal University, Qufu City, Shandong Province 273165, China

## ARTICLE INFO

### Article history:

Received 26 January 2017

Received in revised form 12 June 2017

Accepted 30 June 2017

Available online 2 July 2017

### Keywords:

*o*-Phenylenediamine

Ag<sup>+</sup> ions

Biothiols

Cysteine

Homocysteine

Glutathione

## ABSTRACT

In this work, a label-free and sensitive fluorimetric method has been developed for the detections of biothiols including cysteine (Cys), homocysteine (Hcy), and glutathione (GSH), based on the specific biothiol-induced inhibition of the oxidase-like activity of silver ions (Ag<sup>+</sup>). It is well established that *o*-phenylenediamine (OPD) can be oxidized by Ag<sup>+</sup> ions to generate fluorescent 2,3-diaminophenazine (OPDox). The introduction of biothiols would inhibit the oxidation of OPD by Ag<sup>+</sup> due to the strong coordination between biothiols and Ag<sup>+</sup>. The changes of fluorescence intensities obtained in the Ag<sup>+</sup>-OPD system exhibited good linear correlations in the ranges of 0.50–30.0 μM for Cys, 1.0–45.0 μM for Hcy and 0.50–40.0 μM for GSH. The detection limits (*S/N* = 3) of Cys, Hcy and GSH were 110 nM, 200 nM and 150 nM, respectively. Subsequently, the developed fluorimetric method was successfully applied for the detection of biothiols in human serum.

© 2017 Elsevier B.V. All rights reserved.

## 1. Introduction

Biothiols such as cysteine (Cys), homocysteine (Hcy), and glutathione (GSH) are important components of many proteins and play crucial roles in human physiological functions and pathological conductions [1]. Abnormal levels of biothiols are connected with various chronic diseases, such as arthritis, cancer, HIV/AIDS, and so on [2,3]. For example, deficiency of Cys is usually associated with slowed growth, hair depigmentation, edema, liver damage, lethargy, muscle, and fat loss, and skin lesions etc. [4]. Abnormal Hcy levels are an indicator of chronic renal failure and are associated with cardiovascular disease [5,6]. Also, GSH, as an important antioxidant *in vivo*, plays an important role in physiological processes such as oxidative stress and cell growth [7]. Therefore, it is of great interest to develop efficient methods for the detection of biothiols in biological samples.

During the past decade, a number of effective analytical methods have been developed for the detection of biothiols, typically including high performance liquid chromatography (HPLC) [8], capillary electrophoresis [9], electrochemical method [10], and mass spectrometry (MS) [11,12]. Although these strategies showed promising results for

biothiols detection, there are still some hindrances such as the time-consuming process, the utilization of sophisticated and expensive instrumentation, and the requirement of technical expertise. Recently, fluorescence-based bioanalytical methods have become extremely popular due to their remarkable advantages, such as high sensitivity, simplicity, economy, and real-time detection [13–27]. Particularly, a variety of fluorescent determination methods have been developed for biothiols by using organic dyes [20,21], nanomaterials [22–26] and DNA-based biosensors [27]. However, most of these fluorescent probes used may encounter with the time-consuming preparation procedure and high cost. Therefore, it is still highly desirable to establish more convenient and sensitive assays for biothiols.

Aiming to address the aforementioned drawbacks, we have concentrated on the utilization of conventional yet promising organic fluorophore without the time-consuming synthesis process and complicated post-treatment process. Previous reports have shown that *o*-phenylenediamine (OPD) could be oxidized by Ag<sup>+</sup> ions to yield 2,3-diaminophenazine (usually called OPDox) exhibiting an orange-yellow fluorescence when irradiated by ultraviolet light [28,29]. It is also reported that biothiols possess the strong affinity towards metal cations especially Ag<sup>+</sup> and Hg<sup>2+</sup> [26,27,30,31]. Inspired by these facts, a novel and simple fluorescent assay for biothiols with Ag<sup>+</sup>-regulated and biothiols-inhibited oxidation of OPD has been innovatively developed for the first time. The proposed method is simple and fast for biothiols detection without the complex synthesis procedure and the use of expensive instruments. The developed method was successfully applied to the direct analysis of biothiols in biological fluid.

\* Corresponding author at: Shandong Provincial Key Laboratory of Life-Organic Analysis, College of Chemistry and Chemical Engineering, Qufu Normal University, Qufu City, Shandong Province 273165, China.

E-mail addresses: [shuyunzhu1981@163.com](mailto:shuyunzhu1981@163.com) (S. Zhu), [huawangqfnu@126.com](mailto:huawangqfnu@126.com) (H. Wang).

<sup>1</sup> <http://wang.qfnu.edu.cn>.

## 2. Experimental

### 2.1. Materials and Reagents

Cysteine (Cys), homocysteine (Hcy), glutathione (GSH), AgNO<sub>3</sub>, *o*-phenylenediamine (OPD), Na<sub>2</sub>HPO<sub>4</sub>·12H<sub>2</sub>O, NaH<sub>2</sub>PO<sub>4</sub>·2H<sub>2</sub>O, and 11 other amino acids were purchased from Aladdin Company (Shanghai, China). 10 mM phosphate buffer solutions (PBS) were prepared by mixing stock standard solutions of Na<sub>2</sub>HPO<sub>4</sub> and NaH<sub>2</sub>PO<sub>4</sub>. All reagents were of analytical reagent grade, and used as received. Doubly deionized water was used throughout.

### 2.2. Apparatus

All fluorescence measurements were carried out on a fluorescence spectrophotometer (FluoroMax-4, SPEX, USA) operated at an excitation wavelength at 417 nm. UV–vis spectra were recorded on a UV–vis spectrophotometer (Shimadzu, UV-3600, Japan).

### 2.3. Procedure for the Detection of Biothiols

Cys, Hcy and GSH with different concentrations were freshly prepared before use. First, 5.0 μL of 6.0 mM AgNO<sub>3</sub> were incubated with different concentrations of biothiol solution for a certain time, followed by the addition of 30.0 μL of 6.0 mM OPD for a certain time incubation and then diluted to 500.0 μL with 10 mM PBS at pH 6.0. The fluorescence intensities were recorded in the wavelength range from 450 nm to 700 nm. To investigate the selectivity of this assay, influence of the other 11 amino acids to the Ag<sup>+</sup>-OPD system was investigated. All the fluorescence detection was under the same conditions throughout the experiment: the slit widths of both excitation and emission were 5 nm, respectively.

### 2.4. Determination of Practical Samples

The human serum samples were obtained from the local hospital. For determination of total thiols in serum samples, the disulfide bonds were reduced to the protein-bound thiols by addition of triphenylphosphine (PPh<sub>3</sub>) as catalyst [32,33]. Briefly, 500.0 μL of collected serum were vigorously mixed with 40.0 μL of 0.2 M HCl and 20.0 μL of 0.4 M PPh<sub>3</sub> (in water-acetonitrile 20:80 V/V and 2.0 M HCl). After incubation for 15 min, the hydrolysed serum was mixed with 500.0 μL of acetonitrile to precipitate proteins, followed by centrifugation at 4000 rpm for 20 min. The supernatant containing biothiols in serum was used for further analysis, and the known amount of thiols was estimated using a standard addition method. Since the thiols content of serum is beyond the dynamic range of the proposed method, the serum samples were appropriately diluted with 10 mM PBS before measurement.

## 3. Results and Discussion

### 3.1. Design and Establishment of Biothiols Sensing System

It is well recognized that the aqueous solution of pure OPD was colorless and exhibited negligible fluorescence as shown in Fig. S1. In contrast, the introduction of Ag<sup>+</sup> ions essentially triggered the oxidative reaction of OPD, during which the original colorless and nonfluorescent solution has gradually turned to pale yellow in color and showed intense orange-yellow fluorescent under ultraviolet light. Neither Ag<sup>+</sup> ions nor OPD solution have obvious absorption peak in the visible range, while the Ag<sup>+</sup>-OPD mixed solution has an obvious absorption peak at 417 nm, which belongs to the characteristic absorption spectrum of OPDox, the main oxidation product of OPD [34]. Meanwhile, the corresponding fluorescence excitation peak and emission peak of the Ag<sup>+</sup>-OPD mixed solution were observed at about 417 nm and

560 nm (Fig. S2), respectively, which is similar to that of OPDox in previous work as well [28,29]. Importantly, we found that both the fluorescence and absorption intensities could decrease obviously in the presence of biothiols (Fig. 1B and Fig. S3). This indicated that the oxidative reaction of OPD could be partially inhibited in the presence of biothiols because of the preferential complexation affinity of biothiols to Ag<sup>+</sup>. Thus, the above phenomena illustrate that biothiols could restrain the Ag<sup>+</sup>-OPD oxidative reaction. Therefore, a convenient fluorimetric assay could be designed and established for sensing biothiols sensitively and selectively (Fig. 1A).

### 3.2. Optimization of the Sensing System

The reaction conditions were optimized to establish the optimum analytical conditions. We used the changes of the fluorescence intensities, that is  $F_0-F$ , as a criterion to optimize the detection conditions, where  $F_0$  and  $F$  are the fluorescence intensities at 560 nm in the absence and presence of biothiols, respectively.

#### 3.2.1. Effect of Reaction Time

The effect of reaction time on the detection of biothiols was studied, and the experimental results were shown in Fig. 2. The results indicated that the fluorescence intensity of Ag<sup>+</sup>-OPD system increased gradually and reached the maximum when the reaction time reached 10 min, which means that the oxidation reaction was almost completed within 10 min. However, the fluorescence intensity of Ag<sup>+</sup>-OPD system rapidly decreased in the first 1 min and then changed slightly in the following 15 min upon the addition of biothiols. Obviously, the  $F_0-F$  reached the maximum in 10 min. In the following experiments, reaction time of 10 min was chosen.


#### 3.2.2. Effect of pH Values

The pH value is a crucial factor for almost every sensing system. According to the previous reports, Ag<sup>+</sup> can exhibit excellent oxidation ability towards OPD in acidic media [29]. Thus, we investigated the effects of pH in the range of 4.0–7.0 on the detection of biothiols. As shown in Fig. 3, the Ag<sup>+</sup>-OPD system showed a stronger fluorescence intensity in the weak acidic media (pH 4.0–7.0), whereas the fluorescence intensity of Ag<sup>+</sup>-OPD system decreased obviously in the presence of biothiols. The fluorescence intensity showed the largest difference when the pH value of the media was around 7.0. Therefore, pH 7.0 was the optimal condition for the sensing system.

### 3.3. Sensitivity of the Sensing System

Under the optimization conditions, we evaluated the capability of this analytical system for quantitative detection of biothiols. As shown in Fig. 4, it was clearly seen that with the increase of biothiols concentrations, the fluorescence intensities of Ag<sup>+</sup>-OPD system decreased gradually while the  $F_0-F$  increased systematically. The  $F_0-F$  exhibited a good linear relationship with biothiols in the concentration ranges of 0.50–30.0 μM, 1.0–45.0 μM, and 0.50–40.0 μM for Cys, Hcy, and GSH, respectively. The regression equations were  $F_0-F = 18.99 + 11.22C$  ( $R^2 = 0.9967$ ) for Cys,  $F_0-F = 17.32 + 6.491C$  ( $R^2 = 0.9979$ ) for Hcy, and  $F_0-F = 14.58 + 8.456C$  ( $R^2 = 0.9943$ ) for GSH, respectively. The detection limit ( $S/N = 3$ ) can reach as low as 110 nM, 200 nM and 150 nM for Cys, Hcy and GSH, respectively. Moreover, the repeatability of the proposed method was evaluated by five repeated measurements of 5.0 μM Cys, Hcy and GSH and the relative standard deviation (RSD) was 3.56%, 2.67% and 3.12%, respectively, demonstrating the reliability of the proposed method.

In addition, we compared the characteristics of the proposed sensor with other fluorescent biothiols sensors reported elsewhere. As shown in Table 1, the Ag<sup>+</sup>-OPD system could provide better sensitivity in comparison with DNA-CuNCs [36], CuInS<sub>2</sub> QDs [23], CdTe QDs [22], and diethanol amine modified graphene quantum dots (GQD-DEA) [38].

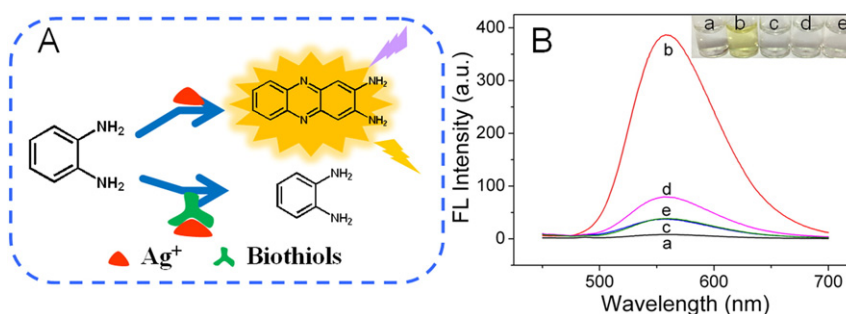


**Fig. 1.** (A) Schematic illustration for the detection of biothiols based on the oxidase-like activity of  $\text{Ag}^+$  ions. (B) Fluorescence emission spectra of OPD (a) and  $\text{Ag}^+$ -OPD system both in the absence and presence of biothiols: (b) No biothiols; (c) 30.0  $\mu\text{M}$  Cys; (d) 45.0  $\mu\text{M}$  Hcy; (e) 40.0  $\mu\text{M}$  GSH. Inset: visual observation of the corresponding solutions.  $[\text{Ag}^+] = 60.0 \mu\text{M}$ ;  $[\text{OPD}] = 360.0 \mu\text{M}$ .

Though the detection limits of the methods using carbon dots [35], DNA-AgNCs [37] and GQDs [25] are lower than that of the developed method, they may entail much longer reaction time to prepare the nanomaterials by using the complicated synthesis and post-treatment process. In contrast, the developed fluorimetric method is relatively simple and fast, and especially using the organic fluorophore that circumvents the time-consuming synthesis process and complicated post-treatment process.

### 3.4. Selectivity of $\text{Ag}^+$ -OPD System for Detecting Biothiols

To verify the performance of our sensor system for biothiols detection in practical applications, we investigated the effects of 11 other common amino acids on the fluorescence intensity of the present sensor system, such as valine (Val), isoleucine (Iso), threonine (Thr), leucine (Leu), phenylalanine (Phe), alanine (Ala), proline (Pro), glycine (Gly), serine (Ser), asparagine (Asn), and methionine (Met). Fig. 5 showed the  $F_0-F$  of the  $\text{Ag}^+$ -OPD system. It could be observed that Cys, Hcy, and GSH exhibited significant changes on the fluorescence intensities of  $\text{Ag}^+$ -OPD system. Other amino acids had more or less positive or negative influences on the sensor system, but no tremendous fluorescence change was observed. These results indicated the proposed method had high selectivity for biothiols and it was practical for the determination of biothiols in biological samples.

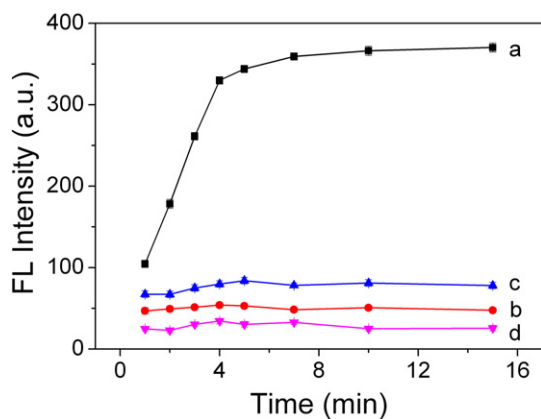


**Fig. 2.** Effects of the reaction time on the fluorescence intensity of the  $\text{Ag}^+$ -OPD system both in the absence and presence of biothiols: (a) no biothiols; (b) 30.0  $\mu\text{M}$  Cys; (c) 45.0  $\mu\text{M}$  Hcy; (d) 40.0  $\mu\text{M}$  GSH.  $[\text{Ag}^+] = 60.0 \mu\text{M}$ ;  $[\text{OPD}] = 360.0 \mu\text{M}$ .

### 3.5. Determination of Biothiols in Serum Samples


The feasibility of the proposed method for practical applications was investigated in the human serum samples. The serum samples were obtained from three healthy adult volunteers with different ages at Qufu peoples' hospital. Because there are a large number of biothiols in serum samples as reported by previous work [39], the concentration of biothiols in human serum was determined by the standard addition method using Cys as the standard. The treated human serum samples were 25-fold diluted by phosphate buffer to ensure that the concentration of biothiols was in the linear range. The obtained concentrations of biothiols in human serum samples were listed in Table 2, which were in agreement with results presented in the literature [40,41]. In addition, Cys was chosen to obtain the recovery of this method since it was the main component of biothiols in human serum. As shown in Table 2, good recoveries (from 94.40% to 111.00%) of the known amounts Cys added to the serum samples demonstrated the reliability of the  $\text{Ag}^+$ -OPD system for detecting biothiols in biological fluids.

## 4. Conclusions

In summary, we have demonstrated a novel, facile, and sensitive fluorimetric method for detection of biothiols based on the inhibition of the  $\text{Ag}^+$  oxidation towards OPD. The protocol shows some excellent advantages of high sensitivity and selectivity for biothiols over various other amino acids. The proposed method is label-free, sensitive, and fast. Moreover, neither nanomaterials nor nucleic acids participated in the assays, making it a simple, cost-effective and lowly laborious

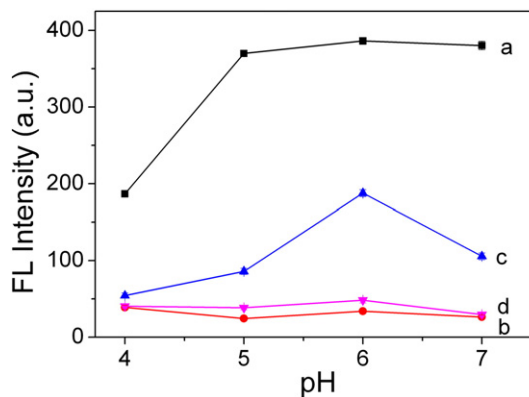

**Fig. 3.** Effect of pH on the fluorescence intensity of the  $\text{Ag}^+$ -OPD system both in the absence and presence of biothiols: (a) no biothiols; (b) 40.0  $\mu\text{M}$  Cys; (c) 40.0  $\mu\text{M}$  Hcy; (d) 40.0  $\mu\text{M}$  GSH.  $[\text{Ag}^+] = 60.0 \mu\text{M}$ ;  $[\text{OPD}] = 360.0 \mu\text{M}$ .

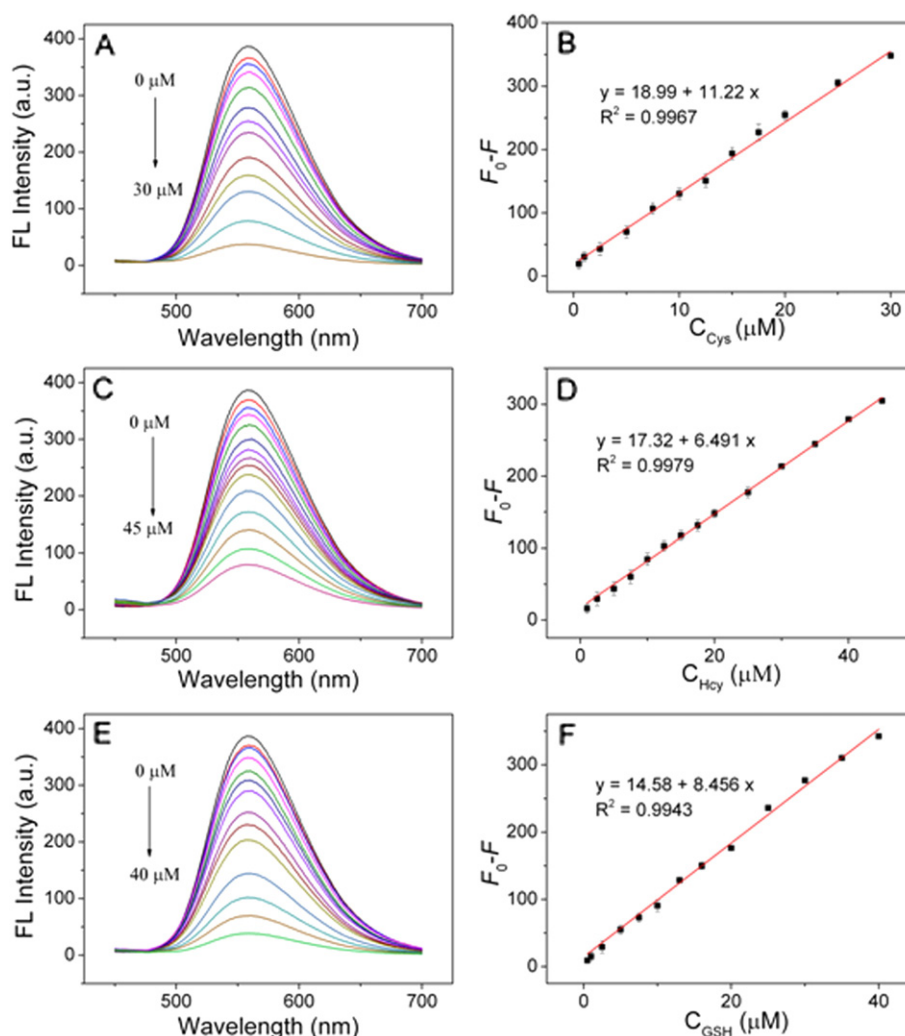

**Fig. 4.** (A) Typical fluorescence spectra of Ag<sup>+</sup>-OPD system in the presence of different amounts of Cys, from top to down: the concentration of Cys is 0, 0.5, 1.0, 2.5, 5.0, 7.5, 10.0, 12.5, 15.0, 17.5, 20.0, 25.0, and 30.0 μM. (B) Relationship between F<sub>0</sub>-F and the Cys concentration. (C) Typical fluorescence spectra of Ag<sup>+</sup>-OPD system in the presence of different amounts of Hcy, from top to down: the concentration of Hcy is 0, 1.0, 2.5, 5.0, 7.5, 10.0, 12.5, 15.0, 17.5, 20.0, 25.0, and 30.0 μM. (D) Relationship between F<sub>0</sub>-F and the Hcy concentration. (E) Typical fluorescence spectra of Ag<sup>+</sup>-OPD system in the presence of different amounts of GSH, from top to down: the concentration of GSH is 0, 0.5, 1.0, 2.5, 5.0, 7.5, 10.0, 13.0, 16.0, 20.0, 25.0, 30.0, 35.0, and 40.0 μM. (F) Relationship between F<sub>0</sub>-F and the GSH concentration.

candidate. More importantly, this method is successfully applied to the determination of biothiols in human serum, indicating its potential in the biological detection or monitoring of the disease biomarkers in the clinical laboratory.

#### Acknowledgements

This work is kindly supported by the National Natural Science Foundation of China (Nos. 21405094, 81303179, and 21675099), the Natural

**Table 1**

Comparison of the detection performances for biothiols among different fluorescent probes.


Probes/Refs	Cys		Hcy		GSH		Synthesis time for probes
	Linear range (μM)	Detection limit (nM)	Linear range (μM)	Detection limit (nM)	Linear range (μM)	Detection limit (nM)	
CDs/[35]	0.01–5	4.9	0.01–5	6.1	0.01–5	8.5	120 min
DNA-CuNCs <sup>a</sup> /[36]	2–100	2000	5–200	5000	2–80	2000	3 min
CuInS <sub>2</sub> QDs <sup>b</sup> /[26]	1–50	500	Not given		Not given		180 min
CdTe QDs-Hg(II)/[22]	2–20	600	Not given		0.6–20	100	Not given
DNA-AgNCs <sup>c</sup> /[37]	0.008–0.1	4	0.6–2	200	0.008–0.1	4	195 min
GQDs/[25]	0–0.125	2.5	0–0.1	5	0–0.05	5	40 min
GQD-DEA/[38]	50–600	10,000	50–100	Not given	100–2000	Not given	24 h
Ag <sup>+</sup> -OPD/ <i>this work</i>	0.5–30	110	1–45	200	0.5–40	150	10 min

<sup>a</sup> Double-strand DNA-templated copper nanoclusters.

<sup>b</sup> Tyrosine-functionalized CuInS<sub>2</sub> quantum dots.

<sup>c</sup> DNA-templated silver nanoclusters.



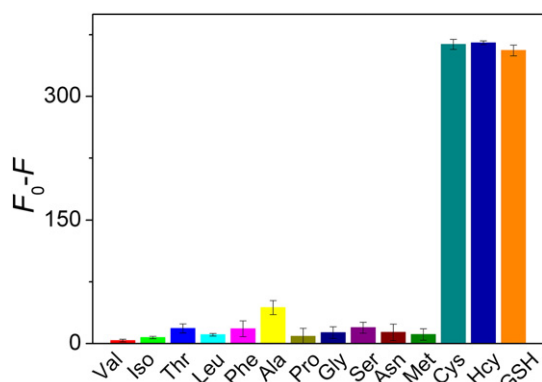

**Fig. 5.** The selectivity of  $\text{Ag}^+$ -OPD system towards various amino acids. The concentration of each amino acid and biothiol is 50.0  $\mu\text{M}$ . Error bars show the standard deviations of three independent experiments.

**Table 2**  
Determination of biothiols in serum samples using the  $\text{Ag}^+$ -OPD reaction system.

Serum sample	Determined biothiols ( $\mu\text{M}$ )	Added Cys ( $\mu\text{M}$ )	Measured ( $\mu\text{M}$ )	Recovery (%)	RSD ( $n = 3, \%$ )
1	292	2.00	1.95	97.50	5.42
		5.00	5.12	102.40	4.65
2	305	2.00	2.12	106.00	3.96
		5.00	4.72	94.40	4.25
3	349	2.00	2.22	111.00	4.25
		5.00	4.91	98.20	3.74

Science Foundation of Shandong Province (No. ZR2013BQ018), the Open Funds of the State Key Laboratory of Electroanalytical Chemistry (No. SKLEAC201506), the National College Students' Innovation and Entrepreneurship Training Program (No. 201610446033), and the Taishan Scholar Foundation of Shandong Province, China.

## Appendix A. Supplementary Data

Supplementary data to this article can be found online at <http://dx.doi.org/10.1016/j.saa.2017.06.056>.

## References

- [1] Z.A. Wood, E. Schroder, J.R. Harris, L.B. Poole, Structure, mechanism and regulation of peroxiredoxins, *Trends Biochem. Sci.* 28 (2003) 32–40.
- [2] J.J. Zhao, K. Zhang, J. Ji, B.H. Liu, Sensitive and label-free quantification of cellular biothiols by competitive surface-enhanced Raman spectroscopy, *Talanta* 152 (2016) 196–202.
- [3] L.A. Herzenberg, S.C. De Rosa, J.G. Dubs, M. Roederer, M.T. Anderson, S.W. Ela, S.C. Deresinski, L.A. Herzenberg, Glutathione deficiency is associated with impaired survival in HIV disease, *Proc. Nat. Acad. Sci. U. S. A.* 94 (1997) 1967–1972.
- [4] S. Shahrokhian, Lead phthalocyanine as a selective carrier for preparation of a cysteine-selective electrode, *Anal. Chem.* 73 (2001) 5972–5978.
- [5] L. Brattström, D.E. Wilcken, Homocysteine and cardiovascular disease: cause or effect? *Am. J. Clin. Nutr.* 72 (2000) 315–323.
- [6] I.J. Perry, R.W. Morris, S.B. Ebrahim, A.G. Shaper, H. Refsum, P.M. Ueland, Prospective study of serum total homocysteine concentration and risk of stroke in middle-aged British men, *Lancet* 346 (1995) 1395–1398.
- [7] J.B. Schulz, J. Lindenau, J. Seyfried, J. Dichgans, Glutathione, oxidative stress and neurodegeneration, *Eur. J. Biochem.* 267 (2000) 4904–4911.
- [8] A.R. Ivanov, I.V. Nazimov, L.A. Baratova, Qualitative and quantitative determination of biologically active low-molecular-mass thiols in human blood by reversed phase high-performance liquid chromatography with photometry and fluorescence detection, *J. Chromatogr. A* 870 (2000) 433–442.
- [9] T. Inoue, J.R. Kirchhoff, Determination of thiols by capillary electrophoresis with amperometric detection at a coenzyme pyrroloquinoline quinone modified electrode, *Anal. Chem.* 74 (2002) 1349–1354.
- [10] W. Wang, L. Li, S.F. Liu, C.P. Ma, S.S. Zhang, Determination of physiological thiols by electrochemical detection with piarselenole and its application in rat breast cancer cells 4T-1, *J. Am. Chem. Soc.* 130 (2008) 10846–10847.
- [11] K.H. Xu, Y. Zhang, B. Tang, J. Laskin, P.J. Roach, H. Chen, Study of highly selective and efficient thiol derivatization using selenium reagents by mass spectrometry, *Anal. Chem.* 82 (2010) 6926–6932.
- [12] B. Seiwert, U. Karst, Simultaneous LC/MS/MS determination of thiols and disulfides in urine samples based on differential labeling with ferrocene-based maleimides, *Anal. Chem.* 79 (2007) 7131–7138.
- [13] N. Zhang, Y.M. Si, Z.Z. Sun, L.J. Chen, R. Li, Y.C. Qiao, H. Wang, Rapid, selective, and ultrasensitive fluorimetric analysis of mercury and copper levels in blood using bimetallic gold-silver nanoclusters with “silver effect”-enhanced red fluorescence, *Anal. Chem.* 86 (2014) 11714–11721.
- [14] S.Y. Li, M.M. Dong, R. Li, L.Y. Zhang, Y.C. Qiao, Y. Jiang, W. Qi, H. Wang, A fluorometric microarray with ZnO substrate-enhanced fluorescence and suppressed “coffee-ring” effects for fluorescence immunoassays, *Nano* 7 (2015) 18453–18458.
- [15] N. Zhang, Y.M. Si, Z.Z. Sun, S. Li, S.Y. Li, Y.H. Lin, H. Wang, Lab-on-a-drop: biocompatible fluorescent nanoparticles of gold nanoclusters for label-free evaluation of phosphorylation-induced inhibition of acetylcholinesterase activity towards the ultrasensitive detection of pesticide residues, *Analyst* 139 (2014) 4620–4628.
- [16] M.M. Dong, C.L. Liu, S.Y. Li, R. Li, Y.C. Qiao, L.Y. Zhang, W. Wei, W. Qi, H. Wang, Polymerizing dopamine onto Q-graphene scaffolds towards the fluorescent nanocomposites with high aqueous stability and enhanced fluorescence for the fluorescence analysis and imaging of copper ions, *Sensors Actuators B Chem.* 232 (2016) 234–242.
- [17] S.Y. Zhu, L. He, F. Zhang, M.Y. Li, S.L. Jiao, Y. Li, M.Y. Chen, X.E. Zhao, H. Wang, Fluorimetric evaluation of glutathione reductase activity and its inhibitors using carbon quantum dots, *Talanta* 161 (2016) 769–774.
- [18] Q. Chen, M. Li, F. Zhang, R. Li, G. Chen, S.Y. Zhu, H. Wang, A turn-on fluorescent probe for phytic acid based on ferric ions-modulated glutathione-capped silver nanoclusters, *Anal. Methods* 8 (2016) 6382–6387.
- [19] Z.Q. Duan, C.X. Zhang, Y.C. Qiao, F.J. Liu, D.Y. Wang, M.F. Wu, K. Wang, X.X. Lv, X.M. Kong, H. Wang, Polyhydric polymer-functionalized fluorescent probe with enhanced aqueous solubility and specific ion recognition: a test strips-based fluorimetric strategy for the rapid and visual detection of  $\text{Fe}^{3+}$  ions, *Talanta* 170 (2017) 306–313.
- [20] W.L. Fang, X.M. Huang, X.M. Shi, Z. Wang, Z.L. Lu, C.H. Fan, Q.B. Bo, A simple fluorescent probe for sensing cysteine over homocysteine and glutathione based on PET, *Spectrochim. Acta A* 173 (2017) 918–923.
- [21] J.X. Dong, X.F. Song, Y. Shi, Z.F. Gao, B.L. Li, N.B. Li, H.Q. Luo, A potential fluorescent probe: Maillard reaction product from glutathione and ascorbic acid for rapid and label-free dual detection of  $\text{Hg}^{2+}$  and biothiols, *Biosens. Bioelectron.* 81 (2016) 473–479.
- [22] B.Y. Han, J.P. Yuan, E.K. Wang, Sensitive and selective sensor for biothiols in the cell based on the recovered fluorescence of the CdTe quantum dots-Hg(II) system, *Anal. Chem.* 81 (2009) 5569–5573.
- [23] S.Y. Liu, F.P. Shi, L. Chen, X.G. Su, Tyrosine-functionalized  $\text{CuInS}_2$  quantum dots as a fluorescence probe for the determination of biothiols, histidine and threonine, *Analyst* 138 (2013) 5819–5825.
- [24] X. Yuan, Y. Tay, X. Dou, Z. Luo, D.T. Leong, J. Xie, Glutathione-protected silver nanoclusters as cysteine-selective fluorometric and colorimetric probe, *Anal. Chem.* 85 (2012) 1913–1919.
- [25] Z.Z. Wu, W.Y. Li, J. Chen, C. Yu, A graphene quantum dot-based method for the highly sensitive and selective fluorescence turn on detection of biothiols, *Talanta* 119 (2014) 538–543.
- [26] L.M. Shen, Q. Chen, Z.Y. Sun, X.W. Chen, J.H. Wang, Assay of biothiols by regulating the growth of silver nanoparticles with c-dots as reducing agent, *Anal. Chem.* 86 (2014) 5002–5008.
- [27] X.L. Yang, W. Wei, J.H. Jiang, G.L. Shen, R.Q. Yu, Conformational switching of G-quadruplexes as a label-free platform for the fluorescence detection of  $\text{Ag}^+$  and biothiols, *Anal. Methods* 8 (2016) 311–315.
- [28] X. Yang, E.K. Wang, A nanoparticle autocatalytic sensor for  $\text{Ag}^+$  and  $\text{Cu}^{2+}$  ions in aqueous solution with high sensitivity and selectivity and its application in test paper, *Anal. Chem.* 83 (2011) 5005–5011.
- [29] H.C. Dai, P.J. Ni, Y.J. Sun, J.T. Hu, S. Jiang, Y.L. Wang, Z. Li, Label-free fluorescence detection of mercury ions based on the regulation of the Ag autocatalytic reaction, *Analyst* 140 (2015) 3616–3622.
- [30] Q.H. Li, L. Zhang, J.M. Bai, Z.C. Liu, R.P. Liang, J.D. Qiu, Preparation of novel fluorescent DNA bio-dots and their application for biothiols and glutathione reductase activity detection, *Biosens. Bioelectron.* 74 (2015) 886–894.
- [31] T. Li, L.L. Shi, E.K. Wang, S.J. Dong, Silver-ion mediated DNAzyme switch for the ultrasensitive and selective colorimetric detection of aqueous  $\text{Ag}^+$  and cysteine, *Chem. Eur. J.* 15 (2009) 3347–3350.
- [32] A.R. Ivanov, I.V. Nazimov, L. Baratova, Determination of biologically active low-molecular-mass thiols in human blood: I. Fast qualitative and quantitative, gradient and isocratic reversed-phase high-performance liquid chromatography with photometric and fluorescence detection, *J. Chromatogr. A* 895 (2000) 157–166.
- [33] L. Shang, S.J. Dong, Sensitive detection of cysteine based on fluorescent silver clusters, *Biosens. Bioelectron.* 24 (2009) 1569–1573.
- [34] S. Fornera, P. Walde, Spectrophotometric quantification of horseradish peroxidase with o-phenylenediamine, *Anal. Biochem.* 407 (2010) 293–295.
- [35] L. Zhou, Y.H. Lin, Z.Z. Huang, J.S. Ren, X.G. Qu, Carbon nanodots as fluorescence probes for rapid, sensitive, and label-free detection of  $\text{Hg}^{2+}$  and biothiols in complex matrices, *Chem. Commun.* 48 (2012) 1147–1149.

- [36] Y.H. Hu, Y.M. Wu, T.T. Chen, X. Chu, R.Q. Yu, Double-strand DNA-templated synthesis of copper nanoclusters as novel fluorescence probe for label-free detection of biothiols, *Anal. Methods* 5 (2013) 3577–3581.
- [37] B.Y. Han, E.K. Wang, Oligonucleotide-stabilized fluorescent silver nanoclusters for sensitive detection of biothiols in biological fluids, *Biosens. Bioelectron.* 26 (2011) 2585–2589.
- [38] D.J. Yu, X.M. Zhang, Y.X. Qi, S.S. Ding, S.M. Cao, A.W. Zhu, G.Y. Shi, Pb<sup>2+</sup>-modified graphene quantum dots as a fluorescent probe for biological aminothiols mediated by an inner filter effect, *Sensor. Actuators B* 235 (2016) 394–400.
- [39] J.P. Richie Jr, L. Skowronski, P. Abraham, Y. Leutzinger, Blood glutathione concentrations in a large-scale human study, *Clin. Chem.* 42 (1996) 64–70.
- [40] L. Shang, J.Y. Yin, J. Li, L. Jin, S. Dong, Gold nanoparticle-based near-infrared fluorescent detection of biological thiols in human serum, *Biosens. Bioelectron.* 25 (2009) 269–274.
- [41] J.V. Ros-Lis, B. Garcia, D. Jimenez, R. Martinez-Manez, F. Sancenon, J. Soto, F. Gonzalvo, M.C. Valdecabres, Squaraines as fluoro-chromogenic probes for thiol-containing compounds and their application to the detection of biorelevant thiols, *J. Am. Chem. Soc.* 126 (2004) 4064–4065.